


SOS Quick Reference Guide
Cardioid Microphones
Plan No 686

Front Triplet Coverage = $90^{\circ} + 90^{\circ}$
Lateral Segment Coverage = 50°
Back Pair Coverage = 80°

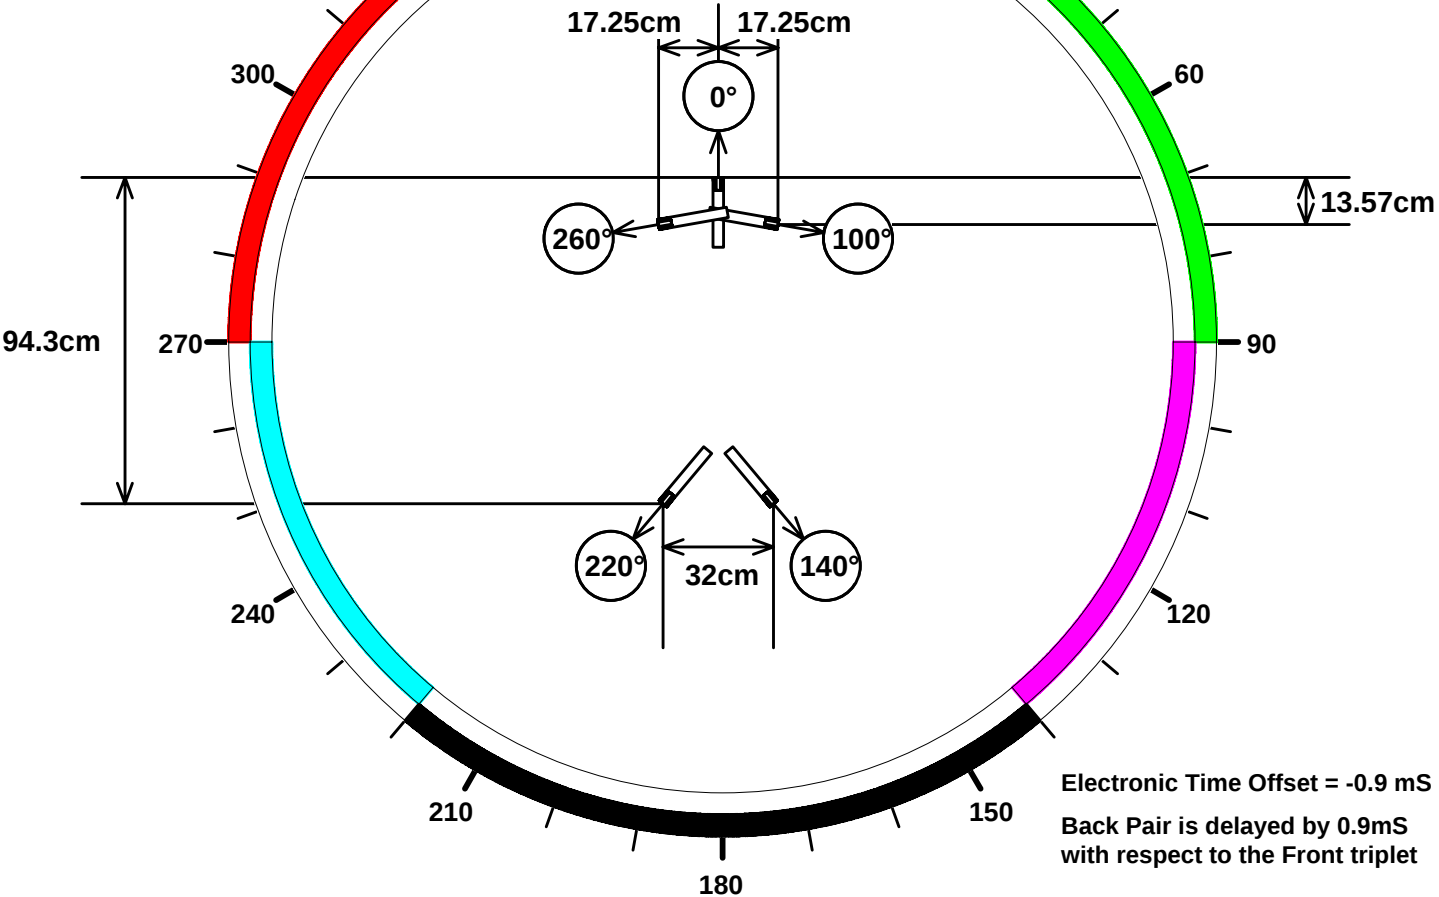

Electronic Time Offset = -0.9 mS
Back Pair is delayed by 0.9mS with respect to the Front triplet